# OMRON

2829552-3B

# Wrist Blood Pressure Monitor

HEM-6181 Instruction Manual



# Table of Contents

Introduction Important Safety Information

# Know Your Monitor

- Preparation Using Your Monitor
- Using Memory Function
- Other Settings
- Error Messages and Troubleshooting Maintenance
- Specifications
- Guidance and Manufacturer's Declaration

### Introduction

Thank you for purchasing the OMRON HEM-6181 Wrist Blood Pressure Monitor. This blood pressure monitor is to be worn on your

This new blood pressure monitor uses the oscillometric method of blood pressure measurement. When the cuff inflates, this monitor senses the pressure pulsations of the artery underneath the cuff. The pulses are called oscillometric pulses. The electronic pressure sensor displays a digital reading of blood pressure.

# Safety Instructions

This instruction manual provides you with important information about the OMRON HEM-6181 Wrist Blood Pressure Monitor. To ensure the safe and proper use of this monitor, READ and UNDERSTAND all of the safety and operating instructions. If you do not understand these instructions or have any questions, contact your local OMRON representative before attempting to use this monitor. For specific information about your own blood pressure, consult with your physician.

### Intended Use

This device is a digital monitor intended for use in measuring blood pressure and pulse rate in adult patient population with wrist circumference ranging from 13.5 cm to 21.5 cm. This monitor detects the appearance of irregular heartbeats during measurement and gives a warning signal with readings. It is mainly designed for general household use.

### Receiving and Inspection

Remove this monitor from the packaging and inspect for damage. If this monitor is damaged, DO NOT USE and consult with your local OMRON representative.

### **Important Safety Information**

Please read the Important Safety Information in this instruction manual before using this monitor.

Please follow this instruction manual thoroughly for your safety. Please keep for future reference. For specific information about your own blood pressure, CONSULT WITH YOUR PHYSICIAN.

Indicates a potentially hazardous situation AWarning which, if not avoided, could result in death or serious injury.

• DO NOT use this monitor on infants, toddlers, children or persons who cannot express themselves.

• DO NOT adjust medication based on readings from this blood pressure monitor. Take medication as prescribed by your physician. ONLY a physician is qualified to diagnose and treat high blood pressure.

• DO NOT use this monitor on an injured wrist or a wrist under medical treatment.

• DO NOT apply the wrist cuff on your wrist while on an intravenous drip or blood transfusion.

 DO NOT use this monitor in areas containing high frequency (HF) surgical equipment, magnetic resonance imaging (MRI) equipment, computerized tomography (CT) scanners. This may result in incorrect operation of the monitor and/or cause

an inaccurate reading DO NOT use this monitor in oxygen rich environments or near flammable gas.

 Consult with your physician before using this monitor if you have common arrhythmias such as atrial or ventricular premature beats or atrial fibrillation: arterial sclerosis: poor perfusion; diabetes; pregnancy; pre-eclampsia or renal disease. NOTE that any of these conditions in addition to patient motion, trembling, or shivering may affect the measurement reading.

• NEVER diagnose or treat yourself based on your readings. ALWAYS consult with your physician.

 This product contains small parts that may cause a choking hazard if swallowed by infants, toddlers or children.

**Battery Handling and Usage** 

· Keep batteries out of the reach of infants, toddlers or children

### Indicates a potentially hazardous situation which, if not avoided, may result in minor or Caution

moderate injury to the user or patient, or cause damage to the equipment or other property. • Stop using this monitor and consult with your physician if

you experience skin irritation or discomfort. · Consult with your physician before using this monitor on a wrist where intravascular access or therapy, or an arteriovenous (A-V) shunt, is present because of temporary interference to blood flow which could result in injury.

 Consult with your physician before using this monitor if you have had a mastectomy. · Consult with your physician before using this monitor if you have severe blood flow problems or blood disorders as cuff inflation can cause bruising.

 DO NOT take measurements more often than necessary because bruising, due to blood flow interference, may occur. • ONLY inflate the wrist cuff when it is applied on your wrist. · Remove the wrist cuff if it does not start deflating during a measurement

• DO NOT use this monitor for any purpose other than measuring blood pressure.

 During measurement, make sure that no mobile device or any other electrical device that emits electromagnetic fields is within 30 cm of this monitor. This may result in incorrect operation of the monitor and/or cause an inaccurate reading.

• DO NOT disassemble or attempt to repair this monitor or other components. This may cause an inaccurate reading. DO NOT use in a location where there is moisture or a risk of water splashing this monitor. This may damage this monitor. • DO NOT use this monitor in a moving vehicle such as in a car.

• DO NOT drop or subject this monitor to strong shocks or vibrations • DO NOT use this monitor in places with high or low humidity or high or low temperatures. Refer to chapter 8.

• Ensure this monitor is not impairing blood circulation by observing the wrist while measurement is occurring. • DO NOT use this monitor in high-use environments such as

- medical clinics or physician offices. • DO NOT use this monitor with other medical electrical (ME) equipment simultaneously. This may result in incorrect operation of the monitor and/or cause an inaccurate reading. Avoid bathing, drinking alcohol or caffeine, smoking.
- exercising and eating for at least 30 minutes before taking a measurement. • Rest for at least 5 minutes before taking a measurement.
- Remove tight-fitting, thick clothing and any accessories from your wrist while taking a measurement. · Remain still and DO NOT talk while taking a measurement.
- ONLY use this monitor on persons whose wrist
- circumference is within the specified range of the cuff. • Ensure that this monitor has acclimated to room temperature before taking a measurement. Taking a measurement after an extreme temperature change could lead to an inaccurate reading. OMRON recommends waiting for approximately 2 hours for the monitor to warm up or cool down when the monitor is used in an environment within the temperature specified as operating conditions after it is stored either at the maximum or at the minimum storage temperature. For additional information of operating and storage/transport temperature, refer to chapter 8.
- DO NOT crease the wrist cuff excessively. • Read and follow the "Correct Disposal of This Product" in chapter 9 when disposing of the device and any used
- accessories or optional parts. • DO NOT use this monitor after the durable period has ended.
- Refer to chapter 8.
- **Battery Handling and Usage** DO NOT insert batteries with their polarities incorrectly
- aligned. • ONLY use 2 "AAA" alkaline batteries with this monitor. DO NOT use other types of batteries. DO NOT use new and used batteries together. DO NOT use different brands of batteries toaether.
- · Remove batteries if this monitor will not be used for a long period of time
- If battery fluid should get in your eyes, immediately rinse with plenty of clean water. Consult with your physician immediately.
- If battery fluid should get on your skin, wash your skin immediately with plenty of clean, lukewarm water. If irritation. injury or pain persists, consult with your physician.
- DO NOT use batteries after their expiration date.
- Periodically check batteries to ensure they are in good working condition
- ONLY use batteries specified for this monitor. Use of unsupported batteries may damage and/or may be hazardous to this monitor.

## 1. Know Your Monitor


# 1.1 Contents

Monitor, 2 "AAA" alkaline batteries, storage case, instruction manual



- a. Wrist cuff
- (Wrist circumference 13.5 cm to 21.5 cm)
- b. Display
- c. Battery compartment d. [Memory] button
- e. [Morning average] button
- [START/STOP] button

## 1.3 Display and Symbols

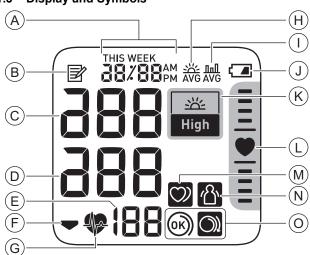


A	Date	and time d	lisplay		2.	Preparation	
в		Memory symbol			2.1	Installing Ba	
			nen viewing readings s	tored in the memory.	1.	Push down the cover and pull	
C D	-		pressure reading				
-			Memory number				
E	When	pressing the proximately o	after the measurement by button, the memory one second before the	ry number appears	2.	Insert 2 "AAA" indicated in the	
F	-	<b>Deflation</b> Appears du	symbol ring cuff deflation.				
G	\$	Heartbeat Flashes wh	: <b>symbol</b> ile taking a measurem	ent.	3	Close the batt	
н	ÄVG	Morning average symbol         3. Close the bat           Appears when viewing the weekly average readings         3.					
I	메 AVG	Appears wh	value symbol nen viewing the averag readings taken within			<b>e</b> /hen the " <b>[</b> " sy ou replace batterie	
J			<b>ymbol (low)</b> en batteries are low.	• Tc Tł	o replace batteries nen replace with 2		
J			<pre>/mbol (depleted) nen batteries are deple</pre>	ted.	da • Re	s soon as batteries ate and time displa eplacing batteries	
к	High	Appears if y	sion symbol rour systolic blood pres or the diastolic blood p		The supplied battery bisposal of used by with local regulation     2.2 Setting the		
	迷 High		nypertension symbolien the morning week	m • As	et your monitor to easurement for th s soon as batterie		
L		<ul> <li>Positioning indicator         Your monitor has a built-in advanced positioning sensor that is used as an aid in determining if the monitor is at the correct height.         The " ● " symbol appears when your monitor is at the correct position relative to your heart during a measurement. When your monitor is higher or lower position relative to your heart, the heart position locator bar will appear up above, or below the heart symbol to guide correct wrist positioning.     </li> <li>Press the (ST, the month, data of the month, data of the month, data of the month, data of the month.</li> </ul>					
М	$\odot$	<ul> <li>Irregular heartbeat symbol</li> <li>Appears along with readings when an irregular rhythm is detected 2 or more times during a measurement.</li> <li>An irregular heartbeat rhythm is defined as a rhythm that is 25% Blood pressure</li> <li>Blood pressure</li> <li>Blood pressure</li> <li>An irregular heartbeat short Long Pulse</li> <li>Blood pressure</li> <li>Blood pressure</li> <li>Blood pressure</li> <li>An irregular heartbeat rhythm detected while your monitor is measuring blood pressure</li> <li>Blood pr</li></ul>					
N	俗	<ul> <li>recommend you to consult with and follow the directions of your physician.</li> <li>Movement error symbol Appears along with readings when your body is moving during a measurement. If it appears, remove the wrist cuff, and wait for 2 to 3 minutes. Then, remain still and</li> <li>2.3 Blood</li> </ul>				e you need to reset nd hold the () b nd time as above Blood Press	
0	Cuff wrap guide symbol (OK)     Appears if the wrist cuff is wrapped around the wrist     correctly while taking a measurement. It also appears     when viewing past readings.     Stress rais     stressful ti     Measurem     It is impor     Taking measurement.					elp ensure an act ress raises blood ressful times. easurements sho is important to tak aking measureme	
-	<ul> <li>Cuff wrap guide symbol (loose)</li> <li>Appears if the wrist cuff is not wrapped around the wrist correctly while taking a measurement. It also appears when viewing poet readings</li> </ul>						
irte	erial hy	ypertensio		nagement of e blood pressure levels	• Av	Caution void bathing, drink nd eating for at lea	
			Office	Home	• Re	est for at least 5 n	
Systolic Blood Pressure			≥ 140 mmHg	≥ 135 mmHg			
Diastolic Blood Pressure			≥ 90 mmHg	≥ 85 mmHg			
	Pressure						

These ranges are from statistical values for blood pressure

\* European Society of Hypertension (ESH) and European Society of Cardiology (ESC).

# A Warning

 NEVER diagnose or treat yourself based on your readings. ALWAYS consult with your physician.

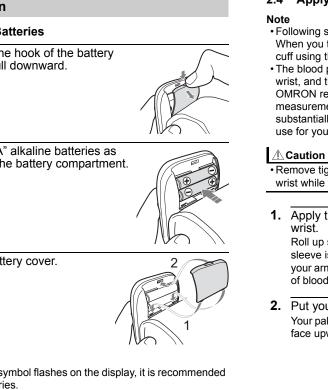

es, turn your monitor off and remove all batteries. 2 new alkaline batteries at the same time. es are correctly installed, the year flashes on the play to set the date and time.


es will not delete previous readings. eries may have a shorter life than new batteries. batteries should be carried out in accordance

# **Date and Time**

to the correct date and time before taking a the first time.

es are correctly installed, the year flashes on the onitor.

or lead button once to adjust the year. the **button** to quickly advance the years. the 👜 button to quickly go backwards through



[ART/STOP] button to store the setting. turns off after 3 seconds.

et the date and time, replace batteries or press button until the year flashes, and set the date steps.

# sure Measurement Tips

ccurate reading, follow these directions: d pressure. Avoid taking measurements during

ould be taken in a quiet place. ake measurements at same times each day. ents in the morning and in the evening is

e a record of your blood pressure and pulse physician. A single measurement does not te indication of your true blood pressure. You record several readings over a period of time

nking alcohol or caffeine, smoking, exercising east 30 minutes before taking a measurement minutes before taking a measurement.


# 2.4 Applying the Wrist Cuff

• Following steps are for applying the wrist cuff to your left wrist.

- When you take a measurement on your right wrist, apply the wrist cuff using the same steps as on your left wrist.
- The blood pressure can differ between the right wrist and the left wrist, and the measured blood pressure values can be different. OMRON recommends to always use the same wrist for measurement. If the values between both wrists differ substantially, please check with your physician as to which wrist to use for your measurements.

• Remove tight-fitting, thick clothing and any accessories from your wrist while taking a measurement.


- 1. Apply the wrist cuff to your left Roll up sleeve. Make sure your sleeve is not rolled up too tightly on your arm. This may constrict the flow of blood in your arm.
- **2.** Put your wrist through the cuff loop. Your palm and monitor display should both face upward.
- **3.** Position the wrist cuff leaving a clearance of 1 to 2 cm between the cuff and the bottom of your palm.



Wrist cuff

4. Wrap the wrist cuff firmly around your wrist. Do not apply over clothing Check to make sure that there is no gap between your wrist and the cuff.


# Note



# 2.5 Sitting Correctly

To take a measurement, you need to be relaxed and comfortably seated in a room with a comfortable temperature. Place your elbow on the table to support your arm.

- Sit in a chair with your leas uncrossed and your feet flat on the floor.
- · Sit with your back and arm being supported.
- Your monitor must be
- approximately the same level as your heart. If the monitor is
- too high above your heart, your blood pressure will be artificially low. If the monitor is too low below your heart, your blood pressure will be artificially high
- Relax your wrist and hand. Do not bend your wrist back, clench your fist, or bend your wrist forward.







# 3. Using Your Monitor

# 3.1 Taking a Measurement

Note

• To stop the measurement, press the [START/STOP] button once to deflate the wrist cuff.


# **∆**Caution

• DO NOT use this monitor with other medical electrical (ME) equipment simultaneously. This may result in incorrect operation of the monitor and/or cause an inaccurate reading. Remain still and DO NOT talk while taking a measurement.

- 1. Press the [START/STOP] button. All symbols appear on the display before starting the measurement.
- 2. Check the positioning indicator.

Your monitor has a built-in advanced positioning sensor that is used as an aid in determining if the monitor is at the correct height. It has been designed to work with most people so that when your wrist is at the correct position relative to your heart,

the " • " symbol will appear. When your wrist is higher or lower position relative to your heart, a locator bar will appear according to the wrist position. Due to difference in individual size and physique, this feature may not be helpful in all cases and you may wish to disable this feature. If you feel the position of the wrist according to positioning indicator's guidance does NOT match your heart level, disable this feature and follow your judgement. To disable it, refer to section 5.1.



	Monitor height	Positioning indicator
	Wrist is too high	Any locator bar (-) above the " $\overline{\Phi}$ " symbol appears.
	Proper position	The " 👿 " symbol appears.
Ξ	Wrist is too low	Any locator bar (-) below the " — " symbol appears.

### Note

• After 5 seconds from pressing the [START/STOP] button, even if your monitor is not positioned properly, your monitor will start the measurement and the wrist cuff will start to inflate.

**3.** Remain still and do not move or talk until the entire measurement process is completed. As the cuff inflates, your monitor automatically determines your ideal inflation level. This monitor detects your blood pressure and pulse rate during inflation.

The " 🏶 " symbol flashes at every heartbeat.

- Note
- The " (iv) " symbol appears if the wrist cuff is wrapped around the wrist correctly.
- When the " 🕥 " symbol is displayed, the wrist cuff is not applied correctly. Press the [START/STOP] button to turn your monitor off, then apply the cuff correctly.

### After your monitor has detected your blood pressure and pulse rate, the cuff automatically deflates. Your blood pressure and pulse rate are displayed.

If either the systolic or the diastolic reading is high (refer to section 1.3), the "High " symbol appears.




# 4. Press the [START/STOP] button to turn your monitor off.

· Your monitor will automatically turn off after 2 minutes. • Wait 2-3 minutes between measurements. The wait time allows the arteries to decompress and return to their premeasurement form. You may need to increase the wait time depending on your individual physiological characteristics.

# 4. Using Memory Function

Your monitor automatically stores up to 60 readings

4.1 Viewing the Readings Stored in Memory





The Memory number appears for one second before the pulse rate is displayed. The most recent reading set is numbered "1".

---

<u>ЛлШ</u> AVG

Ť

88

84

-82

- -

### Note • If the positioning indicator is enabled, the positioning

- indicator is displayed with the readings
- If the reading is high (refer to section 1.3), the "High" symbol appears
- If there are no readings stored in the
- memory, the screen to the right is displayed. • If the memory is full, the monitor will delete the oldest readings.

# **2.** Press the button repeatedly to scroll through the previous readings stored in the memory.

# 4.2 Viewing the Average Reading

Your monitor can calculate an average reading based on the latest 2 or 3 readings taken within 10 minutes span.

1. When your monitor is off, press and hold the 🕞 button for more than 2 seconds.

## Note

- If there are only 2 readings in the memory for that period, the average will be based on these 2 readings.
- If the average reading is high (refer to section 1.3), the "High" symbol appears.

### 4.3 Viewing Morning Weekly Averages Your monitor calculates and displays weekly averages for the


measurements taken in the morning for 4 weeks.

### 1. Press the 🖾 button once. The morning weekly average for the current

- week "THIS WEEK" appears on the display. If the morning weekly average is high (refer to section 1.3), the "
- **2.** Press the button repeatedly to display the average for the previous weeks. Your monitor displays "-1 WEEK" for the previous week's
  - average, to "-3 WEEK" for the oldest set of averages.
- 3. Press the [START/STOP] button to turn off your monitor.


# Morning Weekly Average Calculation

This is the average for the measurements taken during the morning (4:00am - 9:59am) between Sunday and Saturday. Only the first 3 measurements taken in the morning between 4:00am - 9:59am will be used to calculate the morning average for each day.



# 5. Other Settings

- 5.1 Disabling/Enabling Positioning Indicator
- The positioning indicator is enabled as default
- **1.** When your monitor is off, press and hold the 👜 button for more than 10 seconds.





Note Your monitor will automatically turn off after 3 seconds from the completion · To enable the positioning indicator, follow the same steps as

- above.
- 5.2 Deleting All Readings Stored in Memory
- **1.** Press the  $\bigcirc$  button, then the " $\bigcirc$  " symbol appears.
- 2. While holding the Ø button down, press and hold the [START/ STOP] button for more ÷ than 2 seconds.

## Note

•All readings will be deleted. You cannot partially delete the readings stored in the memory

# Error Messages and Troubleshooting

In case of any of the below problems occur during measurement, first check that no other electrical device is within 30cm. If the problem persists, please refer to the table below.

Display/ Problem	Possible Cause	Solution	
appears or the	The wrist cuff is not applied correctly.	Apply the wrist cuff correctly, then take another measurement. Refer to section 2.4.	
wrist cuff does not inflate.	Air is leaking from the wrist cuff.	Contact local OMRON representative.	
<b>E B</b> appears	The wrist cuff is overinflated exceeding 300 mmHg.	Do not touch the wrist cuff while taking a measurement.	
<b>EH</b> appears	You move or talk during a measurement. Vibrations disrupt a measurement.	Remain still and do not talk during a measurement.	
ES appears	The pulse rate is not detected correctly.	Apply the wrist cuff correctly, then take another measurement. Refer to section 2.4. Remain still and sit correctly during a measurement.	
appears		If the " 💟 " symbol continues to appear, we recommend you to consult with your physician.	
<b>E</b> appears	Your wrist is moved up and down during a measurement.	Do not move your wrist, then take another measurement. Refer to chapter 3.	
appears	The monitor is malfunctioned.	Press the [START/ STOP] button again. If "Er" still appears, contact local OMRON representative.	
heart symbol The heart symbol in the positioning indicator does not appear and a locator bar does not appear.	The positioning indicator is disabled.	Enable the positioning indicator. Refer to section 5.1.	
flashes	Batteries are low.	Replacing all batteries with 2 new alkaline batteries is recommended. Refer to section 2.1.	
appears or the monitor is turned off unexpectedly during a measurement	Batteries are depleted.	Immediately replace all batteries with 2 new alkaline batteries. Refer to section 2.1.	
No power. Nothing	Batteries are completely depleted.		
appears on the display of the monitor.	Battery polarities are not properly aligned.	Check the battery installation for proper placement. Refer to section 2.1.	
Readings appear too high or too low.	Blood pressure varies constantly. Many factors including stress, time of day, and/or how you apply the wrist cuff, may affect your blood pressure. Review sections 2.3 - 2.5 and chapter 3.		
Any other problems occur.	Press the [START/STOP] button to turn the monitor off, then press it again to take a measurement. If the problem continues, remove all batteries and wait for 30 seconds. Then re- install batteries. If the problem still persists, contact local OMRON representative.		

# 7. Maintenance

7.1 Maintenance below:

• C	hanges	or mod	dificatio
V	oid the u	iser wa	arranty.

# 7.2 Storage

Do not store your monitor • If your monitor is wet.

# 7.3 Cleaning

cloth.

monitor and wrist cuff.

# 7.4 Calibration and Service

# 8. Specifications

-
Product description
Model
Display
Cuff pressure range
Blood pressure
measurement range
Pulse measurement
range
Accuracy
Inflation
Deflation
Measurement metho
Operation mode
IP classification
Rating
Power source
Battery life
Durable period (Serv life)
Operating conditions
Storage / Transport
conditions
Weight
Dimensions
Measurable wrist
circumference
Memory
Contents
Protection against
electric shock
Cuff Material

of the	app	lied	р	а

Note

- - requirements of ISO 81060-2:2013.

    - issues during a normal operation.

(			
1			

Measurements of the morning Saturday

# To protect your monitor from damage, please follow the directions

ications not approved by the manufacturer will

• DO NOT disassemble or attempt to repair this monitor or other components. This may cause an inaccurate reading.

Keep your monitor in the storage case when not in use. • Store your monitor in a clean, safe location.

· In locations exposed to extreme temperatures, humidity, direct

sunlight, dust or corrosive vapors such as bleach. • In locations exposed to vibrations or shocks.

· Do not use any abrasive or volatile cleaners.

· Use a soft dry cloth or a soft cloth moistened with neutral soap to clean your monitor and wrist cuff, and then wipe them with a dry

· Do not wash or immerse your monitor and wrist cuff in water. · Do not use gasoline, thinners or similar solvents to clean your

• The accuracy of this blood pressure monitor has been carefully tested and is designed for a long service life.

 It is generally recommended to have the unit inspected every two years to ensure correct functioning and accuracy. Please consult your authorised OMRON dealer or local OMRON representative at the address given on the packaging or attached literature.

8. Specifications	
Draduat description	Wriat Dlaad Drassura Manitar
Product description	Wrist Blood Pressure Monitor
Model	HEM-6181
Display	LCD digital display
Cuff pressure range	0 to 299 mmHg
Blood pressure measurement range	SYS: 60 to 260 mmHg DIA: 40 to 215 mmHg
Pulse measurement	DIA: 40 to 213 mining
range	40 to 180 beats / min.
Accuracy	Pressure: ±3 mmHg Pulse: ±5% of display reading
Inflation	Automatic by electric pump
Deflation	Automatic rapid deflation
Measurement method	Oscillometric method
Operation mode	Continuous operation
IP classification	IP 22
Rating	DC3 V 3.0 W
Power source	2 "AAA" alkaline batteries 1.5V
Battery life	Approximately 300 measurements (using new alkaline batteries)
Durable period (Service life)	5 years
Operating conditions	+10°C to +40°C / 15 to 90% RH (non- condensing) / 800 to 1060 hPa
Storage / Transport conditions	-20°C to +60°C / 10 to 90% RH (non- condensing)
Weight	Approximately 86 g not including batteries
Dimensions	Approximately 93 mm (w) × 62 mm (h) × 20 mm (l) (not including the wrist cuff)
Measurable wrist circumference	13.5 to 21.5 cm
Memory	Stores up to 60 readings
Contents	Monitor, storage case, 2 "AAA" alkaline batteries, instruction manual
Protection against electric shock	Internally powered ME equipment
Cuff Material	Nylon and polyester
Applied part	Type BF (wrist cuff)
Maximum temperature of the applied part	Lower than +48°C

 These specifications are subject to change without notice • In the clinical validation study, K5 was used on 85 subjects for determination of diastolic blood pressure.

This monitor is clinically investigated according to the

• IP classification is degrees of protection provided by enclosures in accordance with IEC 60529. This monitor is protected against solid foreign objects of 12.5 mm diameter and greater such as a finger, and against oblique falling water drops which may cause

• This device has not been validated for use on pregnant patients.

# 9. Guidance and Manufacturer's Declaration CE0197

• This device fulfils the provisions of EC directive 93/42/EEC (Medical Device Directive).

 This blood pressure monitor is designed according to the European Standard EN1060, Non-invasive sphygmomanometers Part 1: General Requirements and Part 3: Supplementary requirements for electromechanical blood pressure measuring systems

• This OMRON product is produced under the strict quality system of OMRON HEALTHCARE Co., Ltd., Japan. The Core component for OMRON blood pressure monitors, which is the Pressure Sensor, is produced in Japan.

Symbols description		
Ŕ	Applied part - Type BF Degree of protection against electric shock (leakage current)	
IP XX	Ingress protection degree provided by IEC 60529	
CE	CE Marking	
SN	Serial number	
X	Temperature limitation	
	Humidity limitation	
( <b>-</b> )	Atmospheric pressure limitation	
Ĩ	Need for the user to consult this instruction manual.	
13.5-21.5cm	Indicates the correct positioning for the monitor on the wrist Measurable wrist circumference	
	Battery	
	Direct current	

# Important information regarding Electro Magnetic Compatibility (EMC)

HEM-6181 manufactured by OMRON HEALTHCARE Co., Ltd. conforms to EN60601-1-2:2015 Electro Magnetic Compatibility (EMC) standard. Further documentation in accordance with this EMC standard is available at http://www.omronhealthcare-ap.com/emc-information. Refer to the EMC information for HEM-6181 on the website

**Correct Disposal of This Product (Waste Electrical & Electronic** Equipment)

should not be disposed of, with other household wastes at the end of its working life. To prevent possible harm to the environment or human health from uncontrolled waste disposal, please separate this product from other types of wastes and recycle it responsibly to promote the sustainable reuse of material resources

This marking shown on the product or its literature, indicates that it



Household users should contact either the retailer where they purchased this product, or their local government office, for details of where and how they can return this item for environmentally safe recycling.

Business users should contact their supplier and check the terms and conditions of the purchase contract. This product should not be mixed with other commercial vaste for disposal

Manufacturer	OMRON HEALTHCARE Co., Ltd. 53, Kunotsubo, Terado-cho, Muko, KYOTO, 617-0002 JAPAN
EU-representative	OMRON HEALTHCARE EUROPE B.V. Scorpius 33, 2132 LR Hoofddorp, THE NETHERLANDS www.omron-healthcare.com
Asia Pacific HQ	OMRON HEALTHCARE SINGAPORE PTE LTD. 438A Alexandra Road, #05-05/08 Alexandra Technopark, Singapore 119967 www.omronhealthcare-ap.com
Production Facility	OMRON HEALTHCARE MANUFACTURING VIETNAM CO., LTD. Binh Duong Province, Vietnam